



# **Installation Instructions for the Chemical Mixer Kits for the *Kodak* AUTOMIXER III PLUS**



**Kodak Home Page  
on Internet**



**Tech Bulletin  
on Intranet**



**Table of Contents**

**PLEASE NOTE**    The information contained herein is based on the experience and knowledge relating to the subject matter gained by Eastman Kodak Company prior to publication.

No patent license is granted by this information.

Eastman Kodak Company reserves the right to change this information without notice, and makes no warranty, express or implied, with respect to this information. Kodak shall not be liable for any loss or damage, including consequential or special damages, resulting from any use of this information, even if loss or damage is caused by Kodak's negligence or other fault.



**Warning**

To avoid hazardous conditions, keep floors and floor coverings around your *Kodak X-Omat* Processors and associated drains clean and dry at all times. Any accumulation of fluids from mixing tanks, drain lines, etc., should be cleaned up immediately. In the event of an accumulation of liquid due to backup, overflow, or other malfunctions of the drain associated with your *Kodak X-Omat* Processor, call a plumber or other contractor to correct any problem with the drain. Kodak accepts no responsibility or liability whatsoever for the serviceability of any drain connected to or associated with a *Kodak X-Omat* Processor. Such drains are the sole responsibility of the customer.



This equipment includes parts and assemblies sensitive to damage from electrostatic discharge. Use caution to prevent damage during all service procedures.



**Important**

Use qualified personnel to service the AUTOMIXER III PLUS.

**Table of Contents**

Description	Page
<a href="#">Service Overview</a> .....	3
<a href="#">Parts List</a> .....	3
<a href="#">Electrostatic Discharge</a> .....	3
<a href="#">Installing the Chemical Mixer Kit</a> .....	4
<a href="#">Installing the SPECIFIC GRAVITY FLOATS</a> .....	4
<a href="#">Installing the KNIVES, NEST, and TEMPLATE</a> .....	8
<a href="#">Adjusting the SPECIFIC GRAVITY FLOAT</a> .....	10
<a href="#">Publication History</a> .....	11

## Section 1: Service Overview

### Parts List

Description	RA	RP	EuropeanR P	D1/F1	Qty
CHEMICAL MIXER KIT includes:	9B8886	9B8887	9B8885	9B8884	1
DEVELOPER NEST	8B6764	8B6764	8B6764	8B6754	1
FIXER NEST	8B6767	8B6767	8B6767	8B6755	1
KNIVES/COUPLING	8B6751	8B6751	8B6751	8B6751	AR##AR = As Required.##
DEVELOPER TEMPLATE	8B6778	8B6768	8B6769	8B6761	1
FIXER TEMPLATE	8B6779	8B6765	8B6766	8B6763	1
DEVELOPER FLOAT	1C7802	1C7802	1C7802	1C7802	1
FIXER FLOAT	1C4907	1C7803	1C7803	1C7803	1
SCREWS	852682	852682	852682	852682	4
Installation Instructions	9B8928	9B8928	9B8928	9B8928	1

## Electrostatic Discharge

### Overview

ESD--electrostatic discharge--is a primary source of:

- product downtime
- lost productivity
- costly repairs


While one cannot feel a static charge of less than 3,500 volts, as few as 30 volts can damage or destroy essential components in electronic equipment.

### Preventive Measures


- Always look for an ESD warning label before doing any procedure involving static-sensitive components such as CIRCUIT BOARDS. All static-sensitive components are marked with bright graphic labels, which frequently include instructions. Follow all label instructions.
- Wear a grounding strap when handling static-sensitive components. Always make certain that the clip remains attached to a properly grounded, unpainted, clean surface.
- Repair static-sensitive components at an ESD-protected work station or use a portable grounding mat. For help in setting up an ESD-protected work station, contact your Kodak representative.
- When moving static-sensitive components from one area to another, insert and transport the components in ESD-protective packaging.

## Section 2: Installing the Chemical Mixer Kit

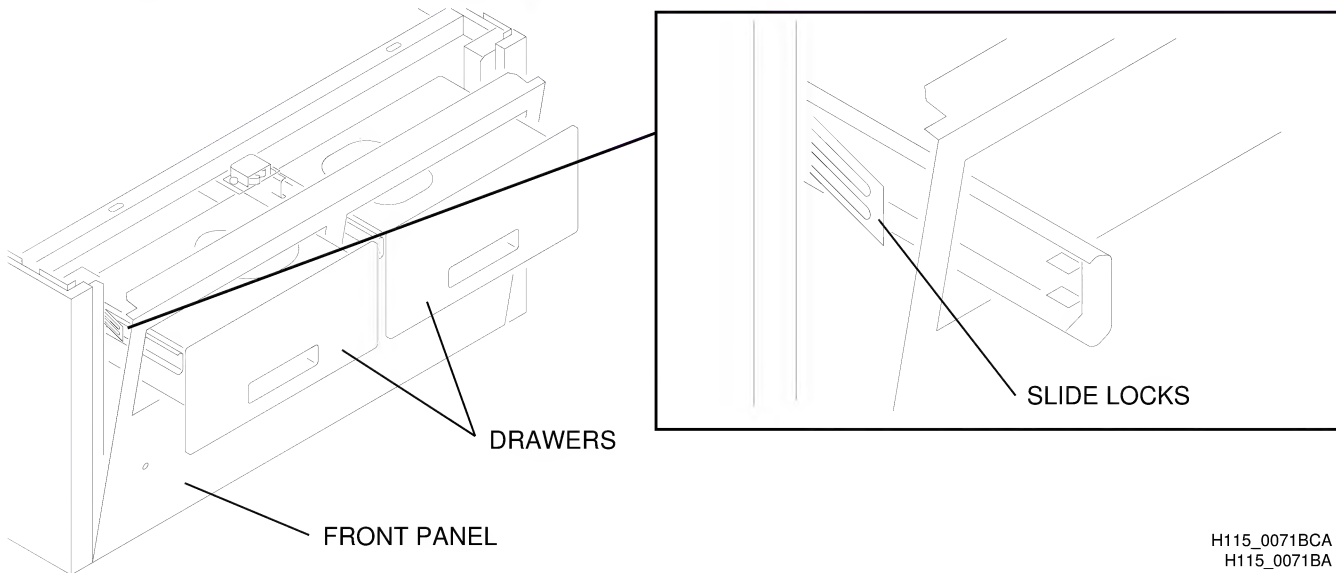

### Installing the SPECIFIC GRAVITY FLOATS

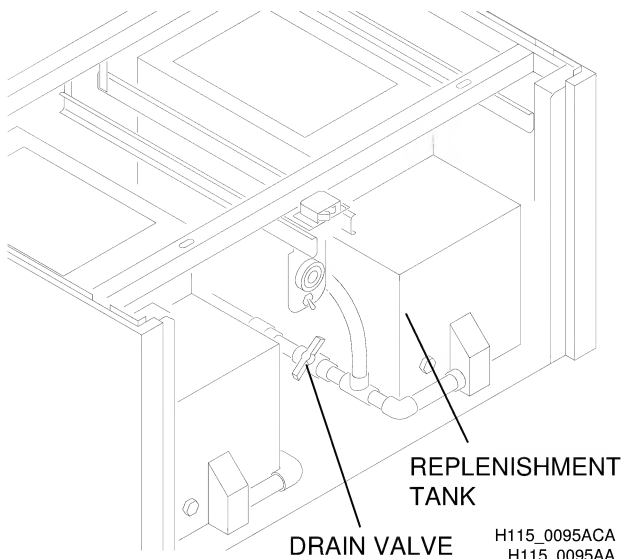


- [1] De-energize the PROCESSOR.
- [2] Turn off the incoming water supply.
- [3] Disconnect the AUTOMIXER.
- [4] Open the 2 DRAWERS.
- [5] For each DRAWER:
  - (a) press the SLIDE LOCKS
  - (b) remove the DRAWER
- [6] Open the FRONT PANEL and disconnect the 2 CONNECTORS P/J5 and P/J8.
- [7] Remove:
  - FRONT PANEL
  - BACK PANEL
  - 2 SIDE PANELS



#### Warning

- Drains must be made of chemically resistant, non-corrosive material. Use PVC or equivalent.
  - The Drain must have a minimum diameter of 7.6 cm (3 in.) and be free of obstruction.
  - Drain service must comply with all local codes.
- [8] Move the DRAIN VALVE  to open the DRAIN.
  - [9] Allow the REPLENISHMENT TANK to drain completely.
  - [10] Move the DRAIN VALVE  to close the DRAIN.

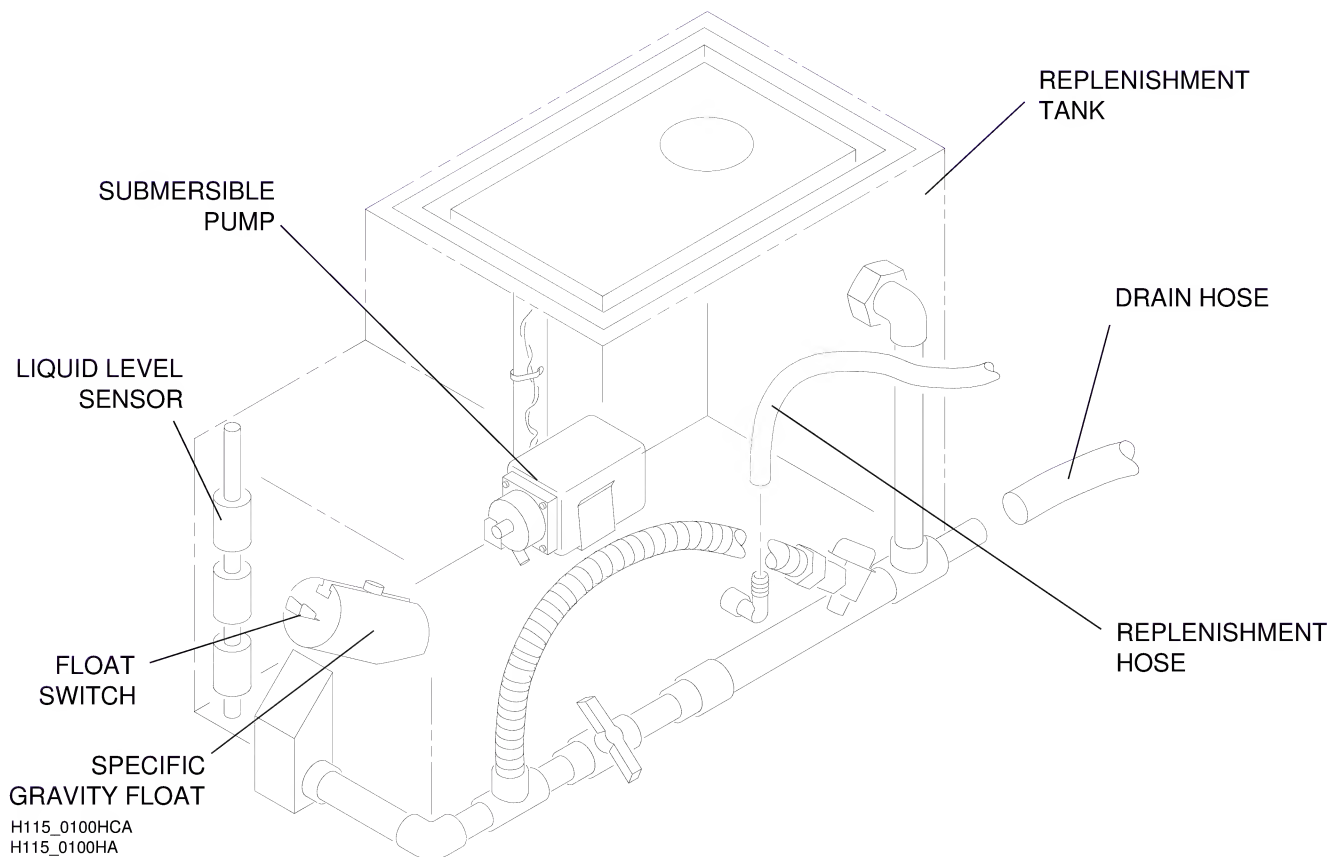


- [11] Disconnect:
- DRAIN HOSE
  - REPLENISHMENT HOSE

[12] Disconnect:

CONNECTOR	Developer	Fixer
FLOAT SWITCH	P/J9	P/J3
LIQUID LEVEL SENSOR	P/J10	P/J2
SUBMERSIBLE PUMP	P/J12	P/J4

- [13] Remove:
- REPLENISHMENT TANK
  - TANK COVER
  - FLOATING LID

SWITCH HINGE PIN

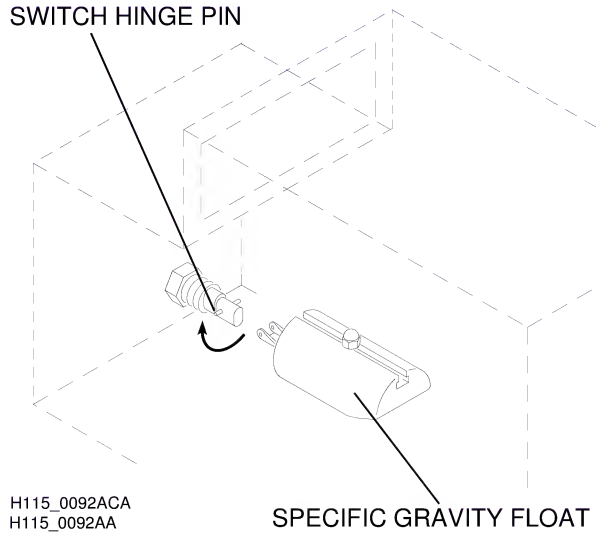

SPECIFIC GRAVITY FLOAT



### Caution

- The SWITCH HINGE PINS break easily. If the SPECIFIC GRAVITY FLOATS are not installed correctly, damage to the SWITCH HINGE PINS can occur.
- Do not move the AUTOMIXER with the SPECIFIC GRAVITY FLOATS installed.

[14] Carefully remove the SPECIFIC GRAVITY FLOAT from the SWITCH HINGE PINS.


[15] Holding the new SPECIFIC GRAVITY FLOAT parallel to the floor of the REPLENISHMENT TANK, engage the SPECIFIC GRAVITY FLOAT on one SWITCH HINGE PIN.


[16] Rotate the SPECIFIC GRAVITY FLOAT carefully until it engages with the other SWITCH HINGE PIN.

[17] Install:

- FLOATING LID
- TANK COVER

TANK COVER

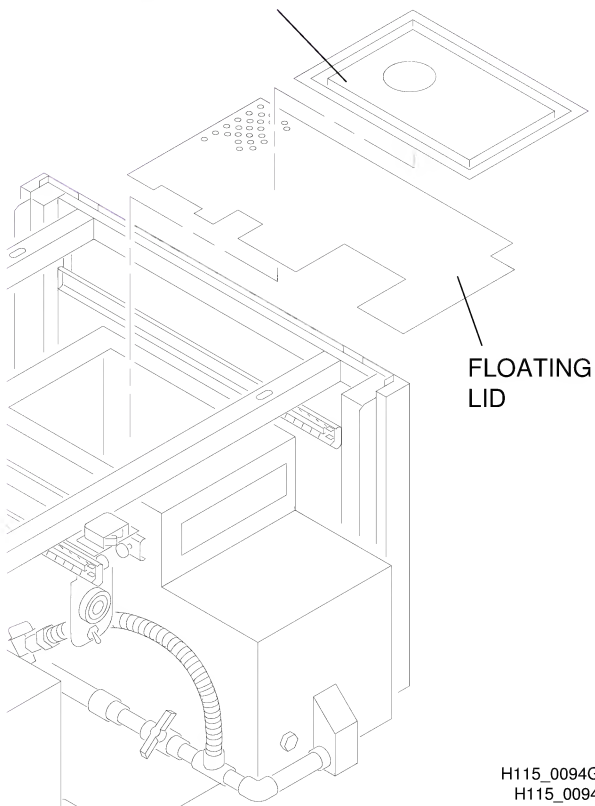

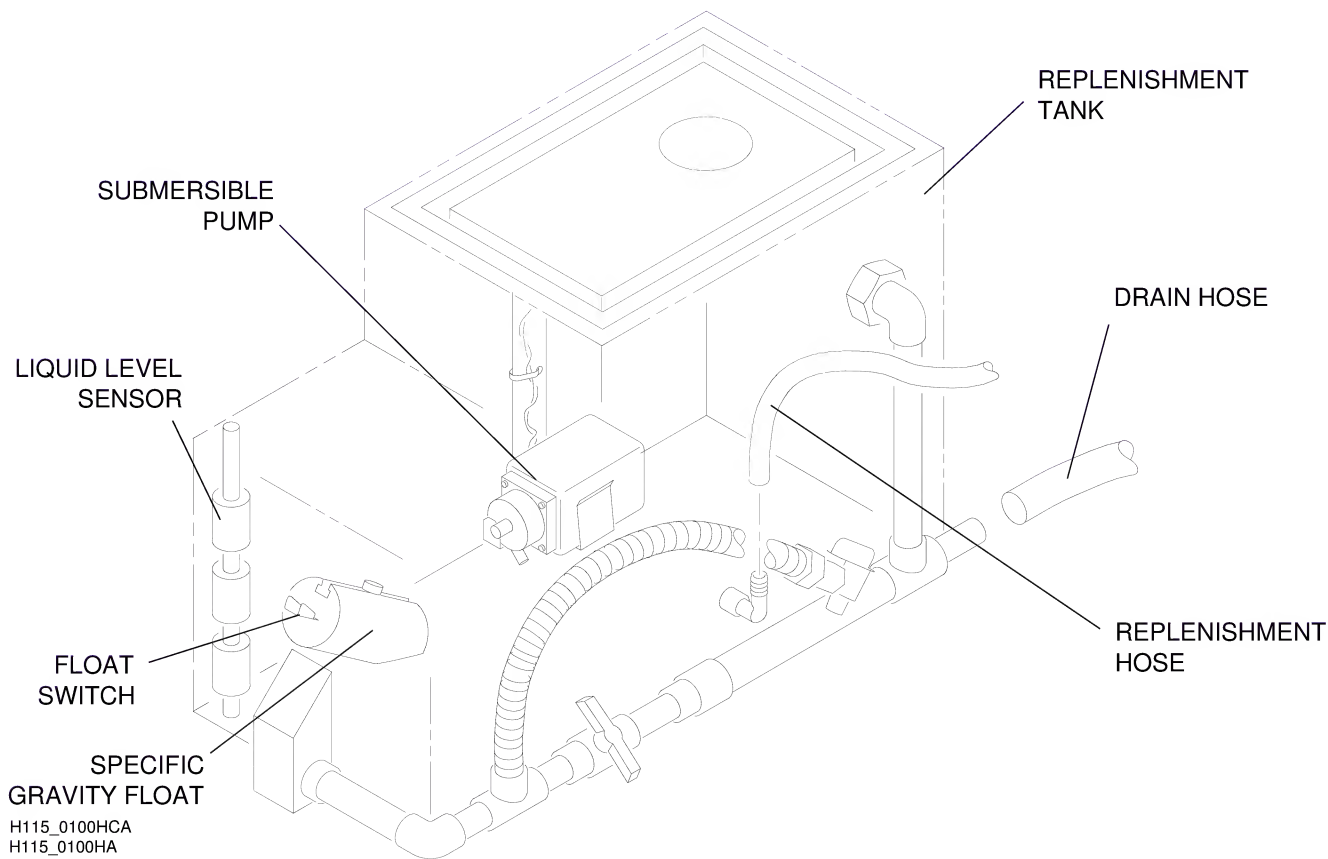


- [18] Connect:
- DRAIN HOSE
  - REPLENISHMENT HOSE

[19] Connect:

CONNECTOR	Developer	Fixer
FLOAT SWITCH	P/J9	P/J3
LIQUID LEVEL SENSOR	P/J10	P/J2
SUBMERSIBLE PUMP	P/J12	P/J4

[20] Install the REPLENISHMENT TANK.

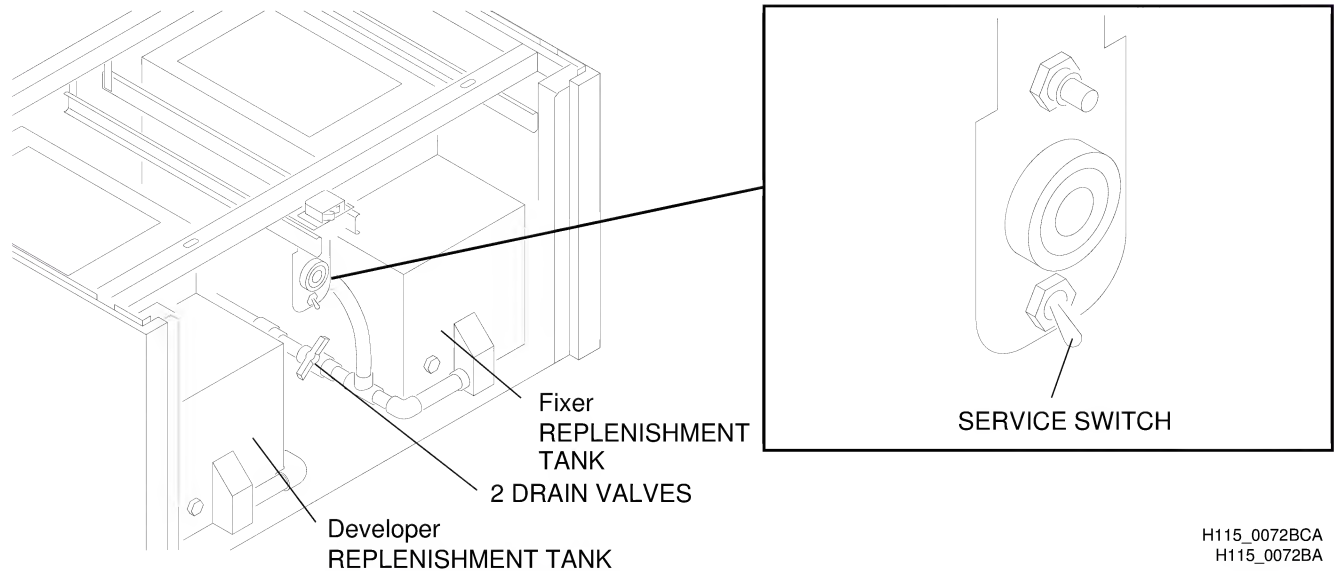


H115\_0072BCA  
H115\_0072BA

## INSTALLATION INSTRUCTIONS

---

- [21] Check that the 2 DRAIN VALVES are closed.
- [22] Connect the AUTOMIXER.
- [23] Turn on the incoming water supply.
- [24] Energize the PROCESSOR.
- [25] Move the SERVICE SWITCH to the left to allow 7.6 cm (3.0 in.) of water to enter into the Developer REPLENISHMENT TANK.
- [26] Move the SERVICE SWITCH to the right to allow 7.6 cm (3.0 in.) of water to enter into the Fixer REPLENISHMENT TANK.

## Installing the KNIVES, NEST, and TEMPLATE

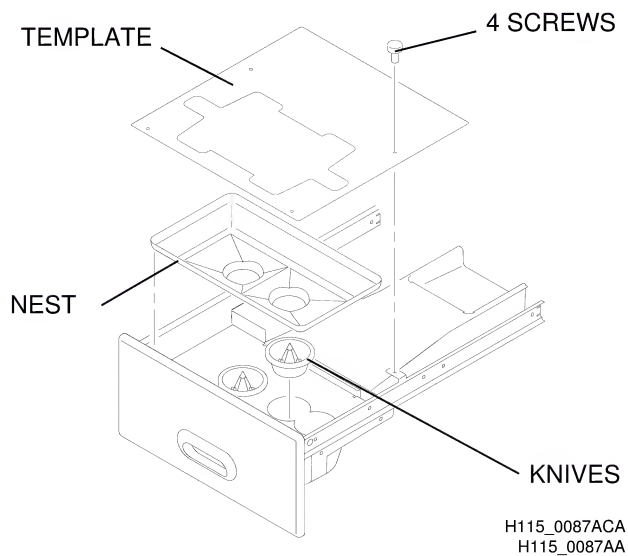


- [1] Remove:
- 4 SCREWS
  - TEMPLATE
  - NEST
  - KNIVES



**Note**

See the figure for the correct configuration of the DRAWERS.

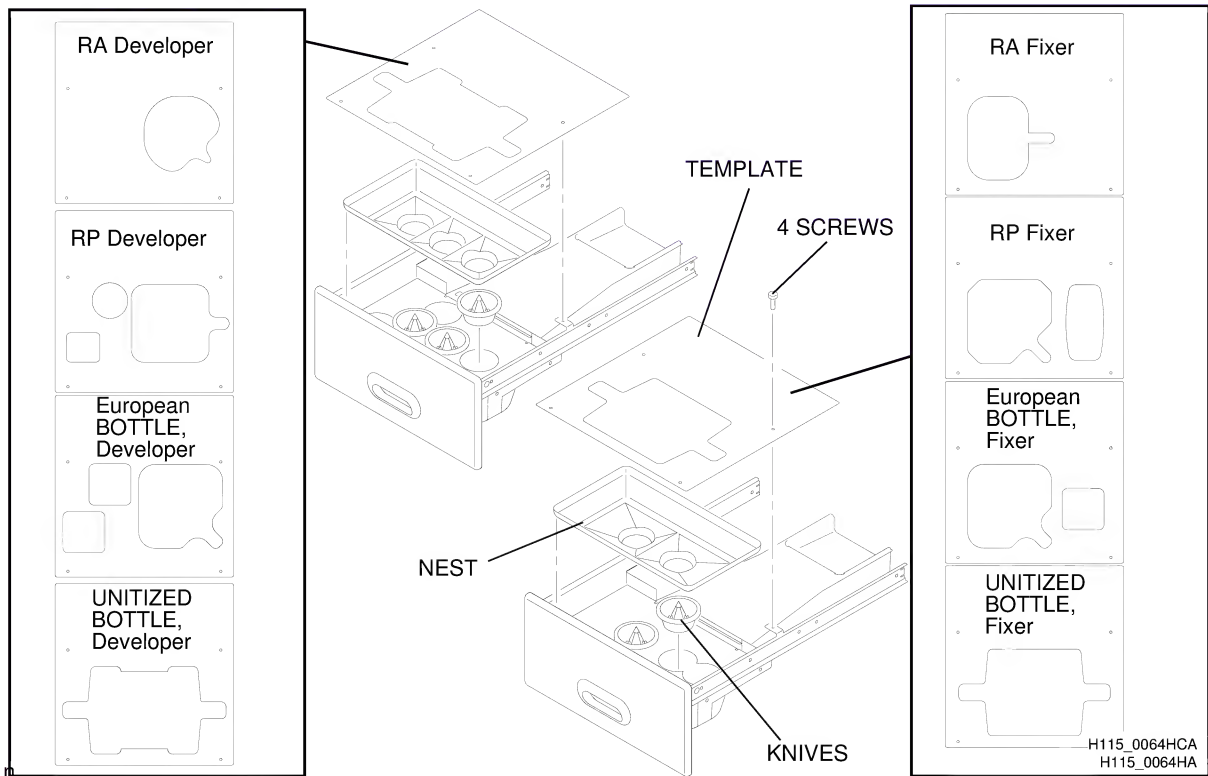

**[2] Install for each DRAWER:**

- KNIVES
- NEST
- TEMPLATE
- 4 SCREWS

**[3] Install:**

- 2 SIDE PANELS
- BACK PANEL
- FRONT PANEL and connect the 2 CONNECTORS P/J5 and P/J8
- 2 DRAWERS

**[4] Check the adjustment for the SPECIFIC GRAVITY FLOAT.**

# Adjusting the SPECIFIC GRAVITY FLOAT

To check:

## Adjustment Specification


Tools: HYDROMETER KIT IC7806



### Important

The following specifications are for the developer and fixer solutions at 21°C (70°F).

- [1] Fill the GRADUATED CYLINDER 3/4 full with the newly mixed solution.
- [2] Place the GRADUATED CYLINDER on a flat surface.
- [3] Insert the HYDROMETER into the GRADUATED CYLINDER.
- [4] Carefully hit the side of the GRADUATED CYLINDER to release any air bubbles from the HYDROMETER.
- [5] Check that the HYDROMETER reads the correct specific gravity:

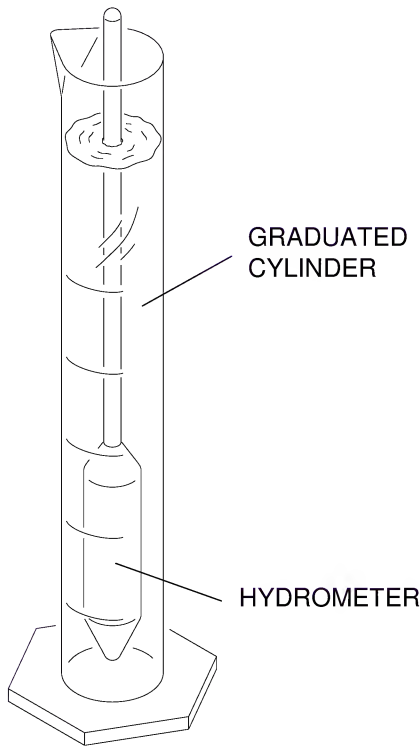


H115\_0008GCA  
H115\_0008GA

SPECIFIC GRAVITY FLOAT	CHEMICAL SOLUTION	SPECIFIC GRAVITY
D-RP	RP Developer	1.085 0.005
D-RA	RA Developer	1.100 0.005
F-RP-LO	RP LO Fixer	1.085 0.005
F-RA	RA Fixer	1.065 0.005

To adjust:

- [1] To increase or decrease the specific gravity of the solution:
  - (a) Loosen the ADJUSTMENT SCREW.
  - (b) Move the ADJUSTMENT SCREW.
  - (c) Tighten the ADJUSTMENT SCREW.

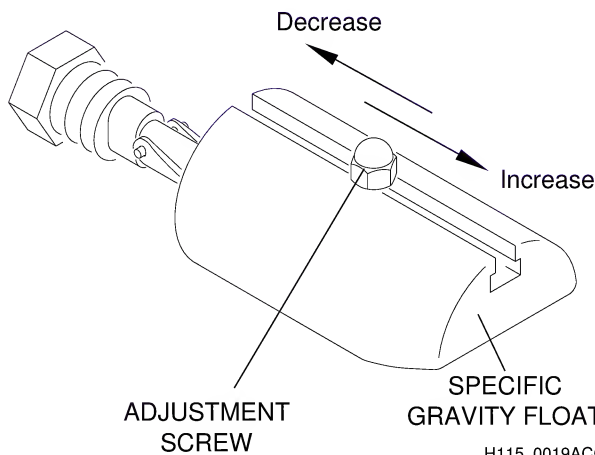

H115\_0019ACC  
H115\_0019AA

---

## Section 3: Publication History

---

Print Date	Pub No.	ECO No.	Affected Pages	File Name	Notes
February 1997	9B8928	2655-001	All	ii3402_001.doc	First Printing

*Kodak and X-Omat are trademarks.*

